



Red Blood Cells deformability index assessment in a hyperbolic microchannel: the diamide and glutaraldehyde effect

Corresponding Author:

Ms. Raquel O Rodrigues,
Research fellow, Mechanics department, Polytechnic Institute of Braganca - Portugal

Submitting Author:

Ms. Raquel O Rodrigues,
Research fellow, Mechanics department, Polytechnic Institute of Braganca - Portugal

Other Authors:

Ms. Vera Faustino,
Research fellow, Mechanics department, Polytechnic Institute of Braganca and CEFT - Portugal
Mr. Elmano Pinto,
Research fellow, Mechanics department, Polytechnic Institute of Braganca and CEFT - Portugal
Ms. Diana Pinho,
Research fellow, Mechanics department, Polytechnic Institute of Braganca and CEFT - Portugal
Dr. Rui Lima,
Professor, Mechanics department, Polytechnic Institute of Braganca - Portugal

Article ID: WMC004375

Article Type: Research articles

Submitted on: 20-Aug-2013, 04:40:16 PM GMT **Published on:** 21-Aug-2013, 02:35:38 PM GMT

Article URL: http://www.webmedcentral.com/article_view/4375

Subject Categories: BIOMEDICAL ENGINEERING

Keywords: Red Blood Cells, Hyperbolic, Microchannel, Diamide, Glutaraldehyde, Deformation

How to cite the article: Rodrigues RO, Faustino V, Pinto E, Pinho D, Lima R. Red Blood Cells deformability index assessment in a hyperbolic microchannel: the diamide and glutaraldehyde effect. WebmedCentral BIOMEDICAL ENGINEERING 2013;4(8):WMC004375

Copyright: This is an open-access article distributed under the terms of the [Creative Commons Attribution License \(CC-BY\)](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Source(s) of Funding:

PTDC/SAU-BEB/108728/2008, PTDC/SAU-BEB/105650/2008, and PTDC/SAU-ENB/116929/2010 from FCT (Science and Technology Foundation), COMPETE, QREN and European Union (FEDER).

Red Blood Cells deformability index assessment in a hyperbolic microchannel: the diamide and glutaraldehyde effect

Author(s): Rodrigues RO, Faustino V, Pinto E, Pinho D, Lima R

Abstract

Red blood cells (RBCs) deformability can be defined as the ability of the cells to deform when subjected to certain flow conditions. In this work, a microfluidic system composed of a microchannel with a hyperbolic-shaped contraction was used to investigate the effect of both diamide and glutaraldehyde on the cell deformation index (DI) of human and ovine RBCs. An adequate image analysis technique was used to measure the DIs of the RBCs travelling in the regions of interest. The results show that the RBCs exposed to diamide and glutaraldehyde decrease their DIs and become more rigid.

Introduction

The red blood cells (RBCs) are the major component of the blood and contain a lot of physiological and clinical information. Hence, there is an increasing interest by the biomedical community as a tool for clinical and biological applications [1,2]. Normal RBCs, at a rest condition, have shapes close to a circle but when they are subjected to certain flow conditions and geometries they have also the ability to undergo strong deformations [3-7]. For example, the RBCs change to an ellipsoid shape when submitted to shear stress and elongate significantly to pass through the smallest capillaries of the microcirculation [8, 9], even when they are smaller than the relaxed discoid cells [10].

The RBC rigidity has been correlated with myocardial infarction, diabetes mellitus, hypertension, and also other haematological disorders and diseases that affect RBC deformation more directly, such as, hereditary spherocytosis, sickle cell anemia, and malaria [4,10]. In *in vitro* environments the RBC rigidity can be induced chemically where diamide and glutaraldehyde are the two most common chemicals used for it [10]. Previous studies have shown that diamide increases the shear modulus and viscosity of the RBC membrane skeleton by creating disulphide bonds preferentially on the spectrin proteins.

Nevertheless, it has little effect on the cytoplasmic or lipid membrane viscosity. For the case of glutaraldehyde, this chemical is a non-specific fixative that promotes the cross-link of the membrane skeletal proteins, phospholipids in the membrane and cytoplasm and consequently it promotes the increase of the shear modulus and viscosity of the entire cell, including the cytoplasm and lipid membrane [11].

Several experimental methods have been used to measure the RBC deformability, such as rheoscopy [3], micropipette aspiration [11, 12], optical tweezers [13], among others. These conventional methods have mainly applied simple shear flows with little focus on extensional flows. Hence, the main objective of the present paper is to measure RBCs deformability index (DI) in a hyperbolic microchannel and examine the effect of both diamide and glutaraldehyde on the cell deformation of human and ovine RBC. For this purpose a hyperbolic microchannel was fabricated and the RBC DI was measured in the extensional flow region by using a high-speed video microscopy system.

Materials and Methods

Physiological working fluids, RBC labeling and microchannel

A standard soft lithography technique was used to fabricate microchannels in polydimethylsiloxane (PDMS) [14, 15]. As described in Illustration 1, the dimension of the microchannel were 400 μm (w) \times 382 μm (l) \times 20 μm (h) where w, l and h refer to the width of the microchannel inlet, length of the hyperbolic contraction region and depth of the microchannel, respectively. As a result the aspect ratio h/w was 0.05. The working fluids used in our experiments was Dextran 40 (Sigma-Aldrich) containing 2% of human RBCs or 2% of ovine RBCs, i. e., haematocrit (Hct) of 2%. The *in vitro* blood used was collected from a healthy donor, where ethylenediaminetetraacetic acid (EDTA) was added to prevent coagulation. All samples were stored hermetical at 4°C until the experiment was performed at room temperature (25 \pm 2°C). Briefly the RBCs were separated from the bulk blood by centrifuging at 2000 RPM for 15min at room

temperature. After removing the buffy coat and plasma, the packed RBCs were then re-suspended and washed twice in physiological salt solution (PSS) 0.9%. For the RBCs exposed to chemicals, the cells were incubated for 10 minutes at room temperature with 0.04% or 0.08% diamide (Sigma-Aldrich) or glutaraldehyde (Sigma-Aldrich). After the incubation time, RBCs exposed to chemicals were washed in PSS 0.9% and re-suspended in Dextran 40 at 2% Hct and then used immediately in our experiments.

Experimental Set-up

The high-speed video microscopy system used in the present study consists of an inverted microscope (IX71, Olympus) combined with a high-speed camera (FASTCAM SA3, Photron). The PDMS microchannel was placed on the stage of the microscope where the flow rate of the working fluids was kept constant (0.5 μ l/min) by means of a syringe pump (PHD ULTRA) with a 1mL syringe (TERUMO® SYRING).

The images of the flowing RBCs were captured using a high speed camera at a frame rate of 7500 frames/s and were then transferred to the computer to be analysed. For each measurement it was taken three sequential videos, in order to make then average.

Image Analysis

The images were processed and analyzed by an image handling software, ImageJ (1.46r, NIH). First, a background image was created from the original stack images by averaging each pixel over the sequence of static images. Next, the background image was subtracted from the original images, resulted in elimination of all the static objects. After that, several image filtering operations such as Median operation were applied to obtain better image quality. Finally, the grey scale images were converted to binary images adjusting the threshold level. The images before and after these processes are shown in Illustration 2.

After the binarization, the flowing RBCs were measured frame by frame manually by using the Analyze Particles function in ImageJ. This way, the major and minor axis lengths of the RBC binary shapes (ellipsoids) were obtained.

Results and Discussion

For all the measurements, major and minor axis lengths of the RBCs were used to determine RBC DI. The formula used to calculate the DI is presented in Illustration 3, where X and Y refer to major and minor axis lengths respectively.

Using a similar approach as Faustino and co-workers

[13], Illustration 4 presents the four sections (S1-S4) where RBC DIs were measured and averaged. Illustration 5 shows the results of DIs for two cases: (a) case 1: human RBCs and (b) case 2: ovine RBCs treated with diamide and glutaraldehyde. Both cases were compared with healthy RBCs not subjected to any treatment. In Illustration 5, from S1 to S3, for all cases, RBCs' DI tends to increase having the maximum value always at S3, which is the region right before the exit of contraction part. At S4, DI dropped down where the cells' shapes start to recover back to its original shape at rest. Based on these results, we have decided to consider S3 as the most suitable region to perform the RBC DIs measurements.

Illustration 6 shows the average and comparison of the two cases investigated in the present study in the region S3. The results show clearly that the RBCs exposed to diamide and glutaraldehyde decrease their DI and become more rigid. This phenomenon happens for both human and ovine RBCs. Moreover, the results show that the RBC deformability tends to reduce as the amount of diamide or glutaraldehyde increases. Another interesting result is that the DIs of human RBCs is always higher when compared with the DIs of ovine RBCs. The main reason for these results may be due to different sizes of the RBCs, i. e., human RBCs are larger than the ovine RBCs, 7.9 and 5.2 μ m respectively [16]. Although the results suggest that the RBC DI differ from specie to specie further detail investigation is currently under way and it will be published in due time.

Illustration 7 represents the decrease of the DI (%) in the region S3 for both cases (human and ovine) when compared with the DI of healthy RBCs subjected not to any kind of treatment. Generally, for the case of human RBCs, glutaraldehyde tend to perform a more effective reduction in the RBC deformability when compared with the effect of diamide. Moreover, the results show that for the case of diamide, the ovine RBCs are the ones which undergo higher reduction in the RBC deformability. Further studies are needed to clarify those phenomena.

Acknowledgment

The authors acknowledge the financial support provided by: PTDC/SAU-BEB/108728/2008, PTDC/SAU-BEB/105650/2008, and PTDC/SAU-ENB/116929/2010 from FCT (Science and Technology Foundation), COMPETE, QREN and European Union (FEDER).

References

1. Kim, D.S., Lee, S.H., Ahn, C.H, Lee, J.Y., Kwon, T.H. (2006) Reusable integrated microfluidic biochip for blood typing by plastic microinjection moulding. *Labchip* 6, 794
2. Lee, S.S., Yim, Y. and Ahn, K.H. (2009) Extensional flow-based assessment of red blood cell deformability using hyperbolic converging microchannel. *Biomed Microdevices* 11, 1021-1027
3. Dobbe J.G.G., Hardeman M.R., Streekstra G.J., Strackee J., Ince C., Grimbergen C.A. (2002) Analysing red blood cell-deformability distribution. *Blood Cells Mol Dis.* 28, 373-384
4. Faustino V., Pinho D., Yaginuma T., Calhelha R., Oliveira M.S.N., Ferreira I., Lima R. (2013) Flow of red blood cells suspensions through hyperbolic microcontractions. In: R. Lima, T. Ishikawa, Y. Imai & M. S. N. Oliveira (Eds), *Visualization and simulations of complex flows in biomedical engineering*, Springer (in press)
5. Yaginuma T, Oliveira MSN, Lima R, Ishikawa T, Yamaguchi T, (2013). Human Red Blood Cell Behavior under Homogeneous Extensional Flow in a Hyperbolic-Shaped Microchannel, (submitted).
6. Pinho D., Yaginuma T, Lima R, (2013). A Microfluidic Device for Partial Cell Separation and Deformability Assessment, (submitted)
7. Leble V, Lima R, Dias R, Fernandes C, Ishikawa T, Imai Y, Yamaguchi T (2011). Asymmetry of red blood cell motions in a microchannel with a diverging and converging bifurcation. *Biomicrofluidics* 5, 044120
8. Hardeman M.R., Ince C. (1999) Clinical potential of in vitro measured red cell deformability, a myth? *Clinical Hemorheology and Microcirculation* 21, 277-284
9. Tong, X. and Caldwell, K.D. (1995) Separation and characterization of red blood cells with different membrane deformability using steric field-flow fraction. *J. Chromatography B.* 674, 39-47
10. Forsyth, A.M., Wan, J., Ristenpart, W.D., Stone, H.A. (2010) The dynamic behaviour of chemically "stiffened" red blood cells in microchannel flows. *Microvascular Research* 80, 37-43
11. Paulitschke, M., Nash, G.B. (1993) Micropipette methods for analysing blood cell rheology and their application to clinical research *Clin. Hemorheol. Microcirc.* 13, 407
12. Shiga T, Maeda N, Kon K. Erythrocyte rheology. *Crit Rev Oncol Hemat* 1990; 10: 9-48
13. Dao, M.C., Lim, T., Suresh, S. (2003) Mechanics of the human red blood cell deformed by optical tweezers. *J. Mech. Phys. Solids* 51, 2259
14. Lima, R., Wada, S., Tanaka, S., Takeda, M., Ishikawa, T., Tsubota, K., Imai, Y. and Yamaguchi, T. (2008). In vitro blood flow in a rectangular PDMS microchannel: experimental observations using a confocal micro-PIV system. *Biomedical Microdevices.* 10, 153-167
15. Lima R, Fernandes C, Dias R, Ishikawa T, Imai Y, Yamaguchi T (2011). Microscale flow dynamics of red blood cells in microchannels: an experimental and numerical analysis. In: Tavares and Jorge (Eds) *Computational Vision and Medical Image Processing: Recent Trends*, Springer 19, 297-309
16. Gregory, R.T. (2000). Nucleotypic effects without nuclei: Genome size and erythrocyte size in mammals. *Genome* 43, 895-901

Illustrations

Illustration 1

The microfluidic channel used to quantify RBC DI. (a) Illustration of the entire microchannel. (b) Dimensions of the hyperbolic microchannel.

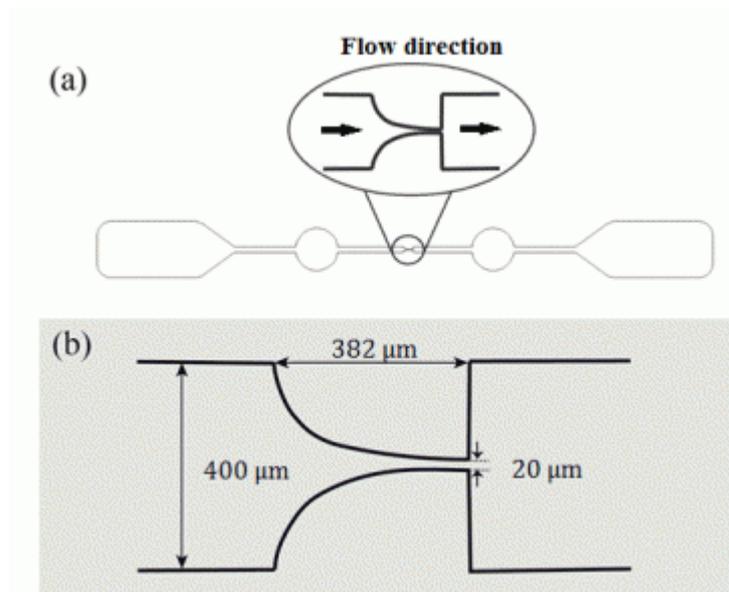


Illustration 2

Steps of image analysis. (a) Original image. (b) Corresponding binary image.

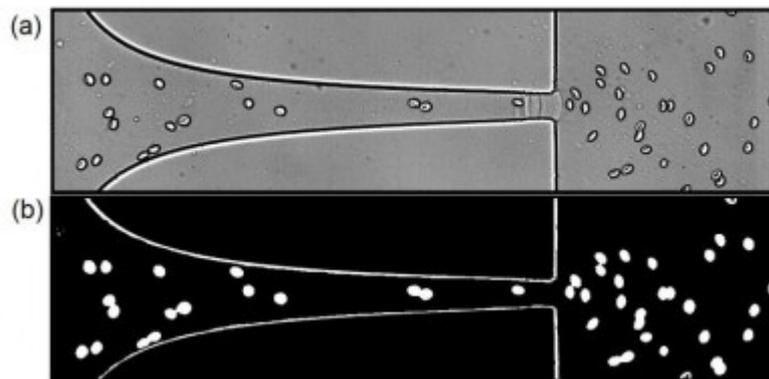


Illustration 3

Definition of the deformation index (DI).

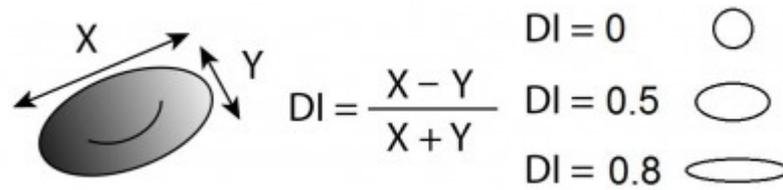


Illustration 4

The four sections used to measure RBC DIs, as well the deformation result of RBCs along the microchannel, adapted from [4].

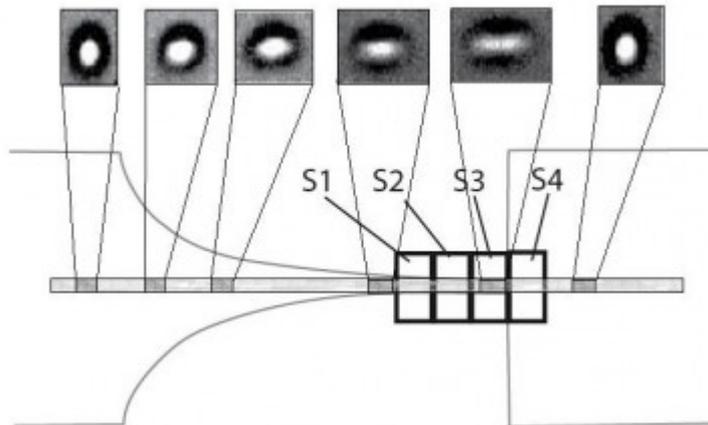


Illustration 5

DI for the four sections studied. (a) Human RBCs and (b) Ovine RBCs, treated with Diamide and Glutaraldehyde, as well as healthy RBCs without chemical treatment.

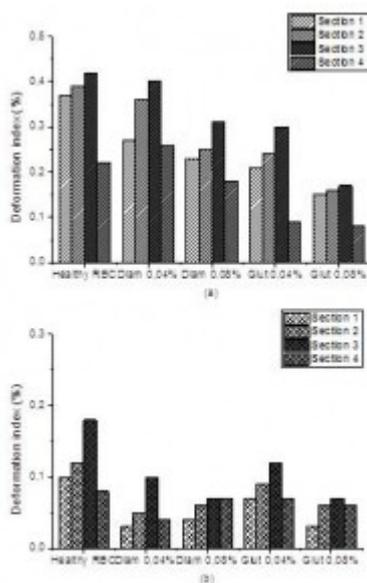


Illustration 6

DI for section S3 for the two cases studied: Case 1, human RBCs; Case 2, ovine RBCs, treated with Diamide and Glutaraldehyde, as well as healthy RBCs subjected to any treatment.


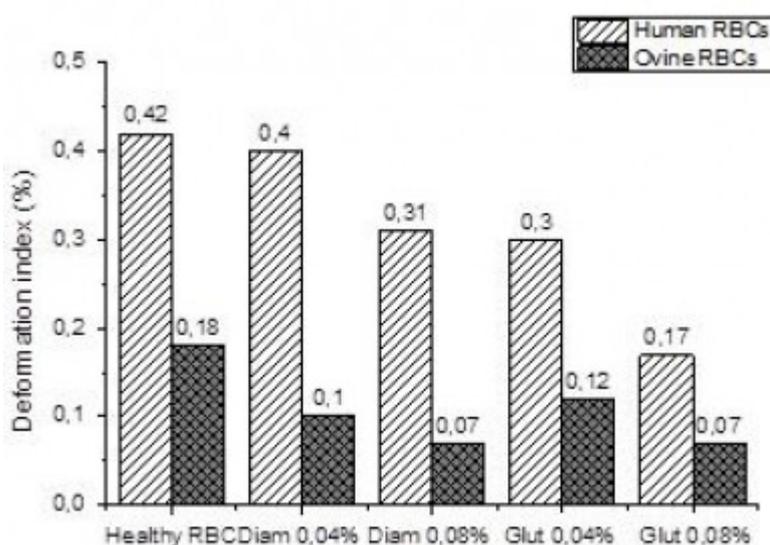


Illustration 7

Decrease of the DI (%) in section S3 for both cases when compared with healthy RBCs subjected to any treatment.

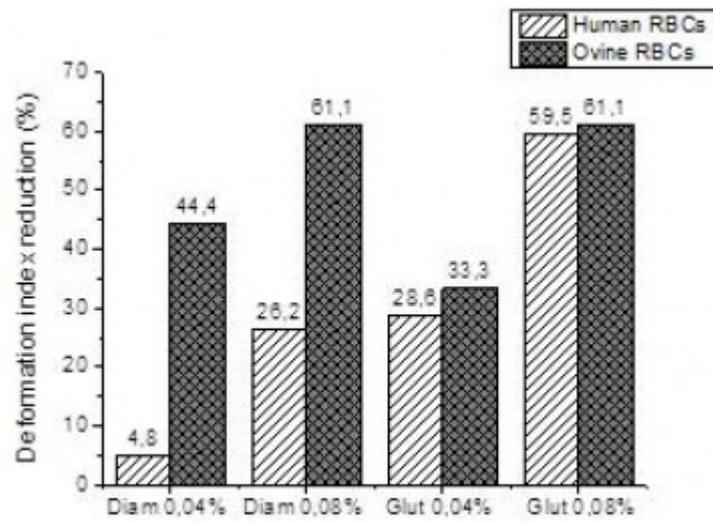

Disclaimer

This article has been downloaded from WebmedCentral. With our unique author driven post publication peer review, contents posted on this web portal do not undergo any prepublication peer or editorial review. It is completely the responsibility of the authors to ensure not only scientific and ethical standards of the manuscript but also its grammatical accuracy. Authors must ensure that they obtain all the necessary permissions before submitting any information that requires obtaining a consent or approval from a third party. Authors should also ensure not to submit any information which they do not have the copyright of or of which they have transferred the copyrights to a third party.

Contents on WebmedCentral are purely for biomedical researchers and scientists. They are not meant to cater to the needs of an individual patient. The web portal or any content(s) therein is neither designed to support, nor replace, the relationship that exists between a patient/site visitor and his/her physician. Your use of the WebmedCentral site and its contents is entirely at your own risk. We do not take any responsibility for any harm that you may suffer or inflict on a third person by following the contents of this website.